


ITEM CODE
SF2461SE

ITEM DESCRIPTION
STANDARD ANGIO PACK II

01 High Pressure Line connecting tube 75cm M/F
01 4 ways Stopcock OFF
01 Manifold 3 port RH RA OFF
02 Infusion set 180cm
01 Scalpel no.11
01 Guidewire J tip 0.035" 150cm single packed
03 Syringe 3ml L.L.
06 Syringe 10ml L.L.
01 Syringe 12ml - 3 rings
02 Syringe 20ml L.L.
03 Syringe 5ml L.L.
02 Hypodermic needle 18G 1 1/2"
03 Hypodermic needle 21G 1 1/2"
02 Hypodermic needle 23G 1 1/2"
02 Hypodermic needle 25G 1"
01 Puncture needle 18G x 7cm
01 Needle Holder Forcep
03 Sponge stick
04 Clamp of towels
05 Blue Towels
07 Laparotomy gauze 50 x 50cm 4ply
40 Gauze 10 x 10 16 ply
02 Reinforced gown XL with towels
02 Bowl 250ml
01 Bowl 500ml
01 Transparent Bowl 100ml
01 Guidewire bowl
02 Kidney bowl 700ml
01 Skin marker
01 Disposable Scissor
01 Label set NTG/Yellow-2, Heparin/Red-2, Normal
01 Table drape 150x180cm
01 Angio drape 250 x 370cm 4 holes
02 Instrument cover 100x80
01 Blue tray 23x31x7 cm

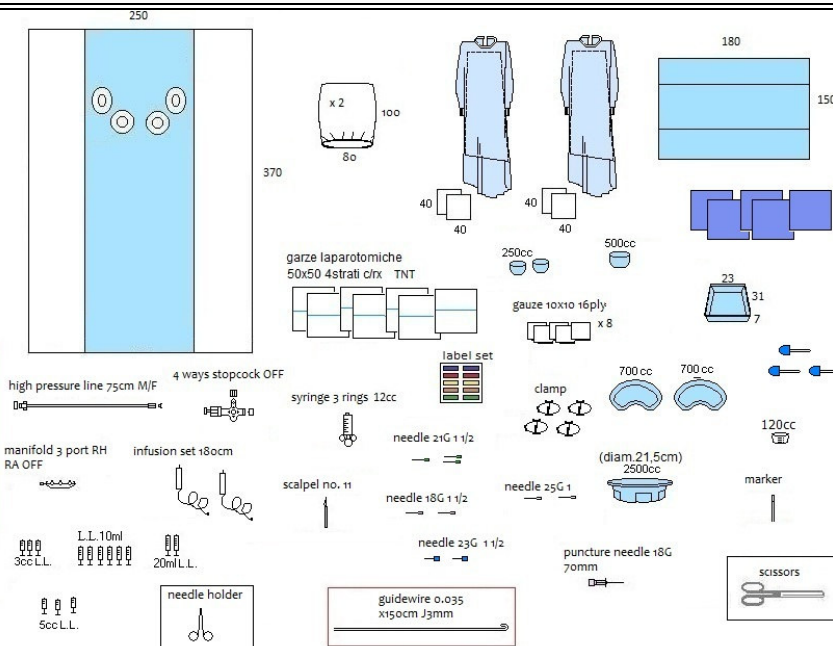

Betatex S.p.A. products are identified by a lot number to refer to

Packing: Boxes of 3 pieces

Sterilization: ETO sterilization

Class: Class IIA Sterile

Intended use: Indicated for Angiography in order to create a barrier to liquids and blink and consequently avoid contamination to the patient.

Allowance: ±3%

QUALITY ASSURANCE

Betatex S.p.A. Assisi adopts a qualità system in compliance with the standard UNI EN ISO 9001:2008 – UNI EN ISO 13485:2004 certified by Det Norske Veritas Italia, CERT registration nr. 11140-2002-AQ-IND SINCERT

The Quality Assurance manual is available on customer's request.

Specific system requirements need to be agreed upon when drawing up the contract

Data sheet nr.	Date of issue	Revision nr.	Date of revision	Created by	Product Engineering Manager	Page
924.671	03/02/2016	2	18/03/2016	Valeria Busti	Simona Sambuchi	1 of 5
Betatex S.p.A. – Viale Europa – 06080 Ospedalicchio di Bastia Umbra (PG) – Italia Tel. +39 (075) 8004872 – Fax +39 (075) 8004972					www.betatex.com info@betatex.com	