


# NHANCER<sup>PRO</sup>X

HYBRID GUIDEWIRE SUPPORT CATHETER

...ENHANCE PRIMARY GUIDEWIRE CROSSING

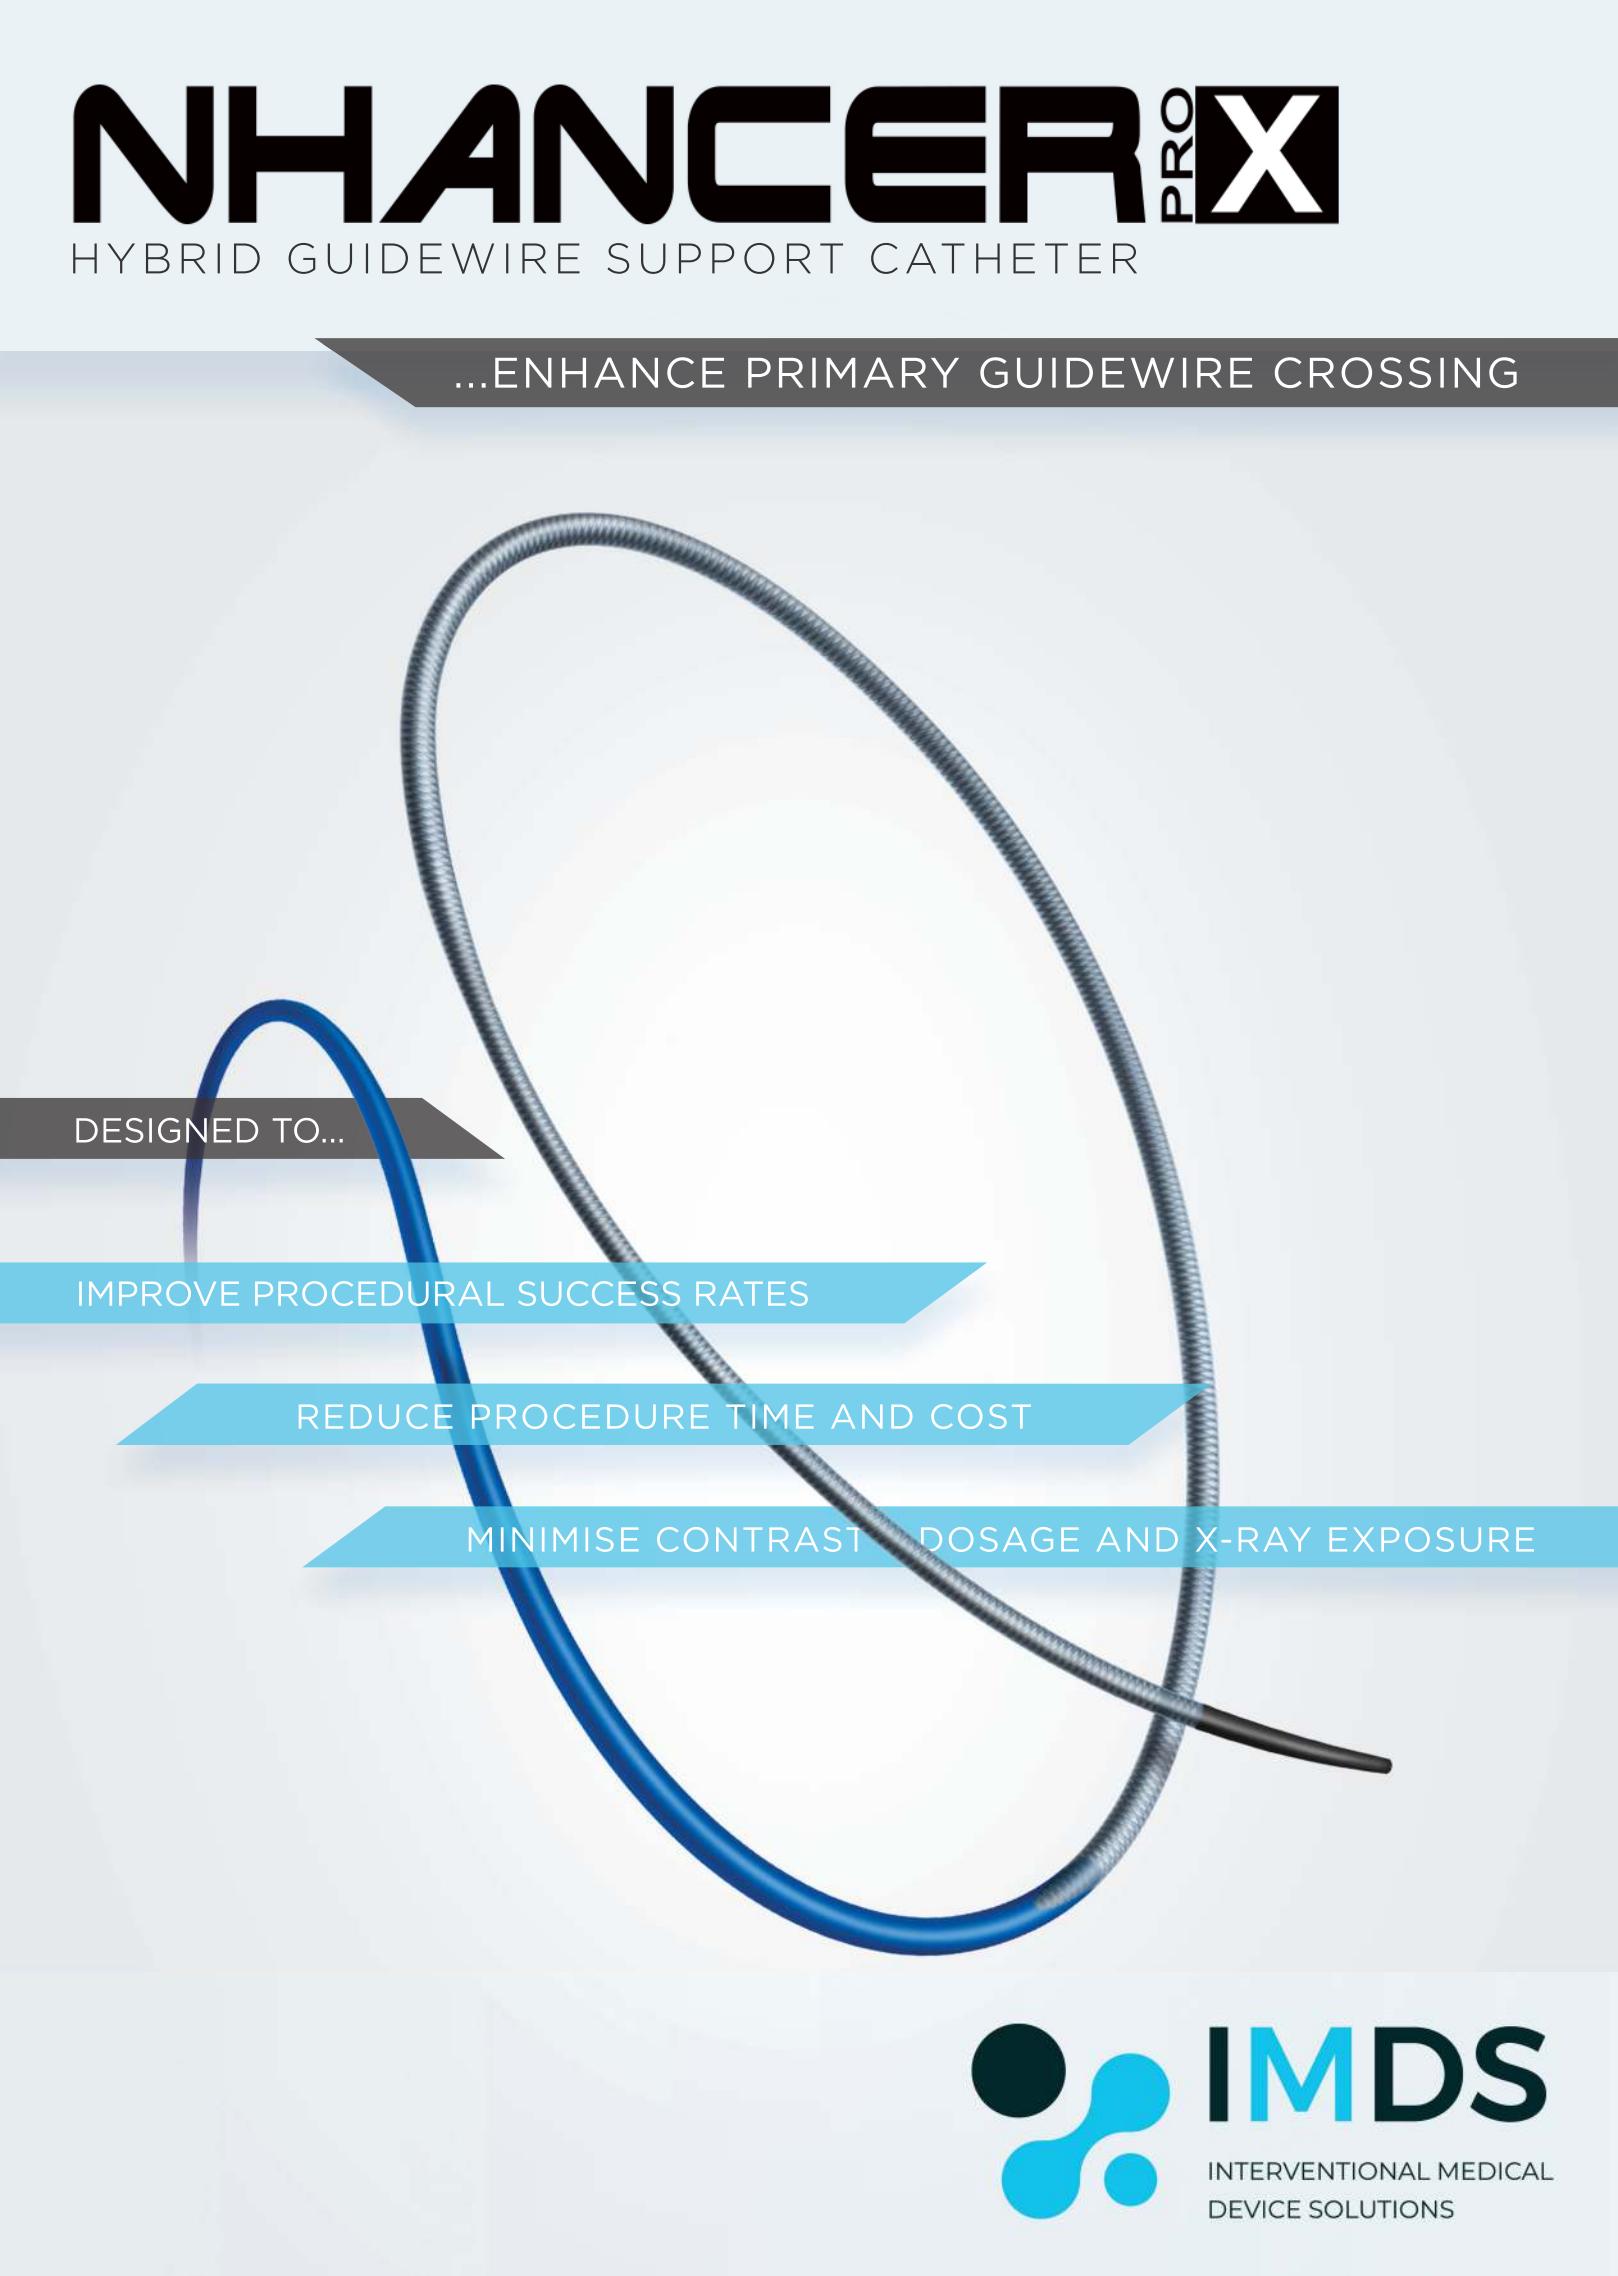

DESIGNED TO...


IMPROVE PROCEDURAL SUCCESS RATES

REDUCE PROCEDURE TIME AND COST


MINIMISE CONTRAST DOSAGE AND X-RAY EXPOSURE

# NHANCER PRO X

## HYBRID GUIDEWIRE SUPPORT CATHETER

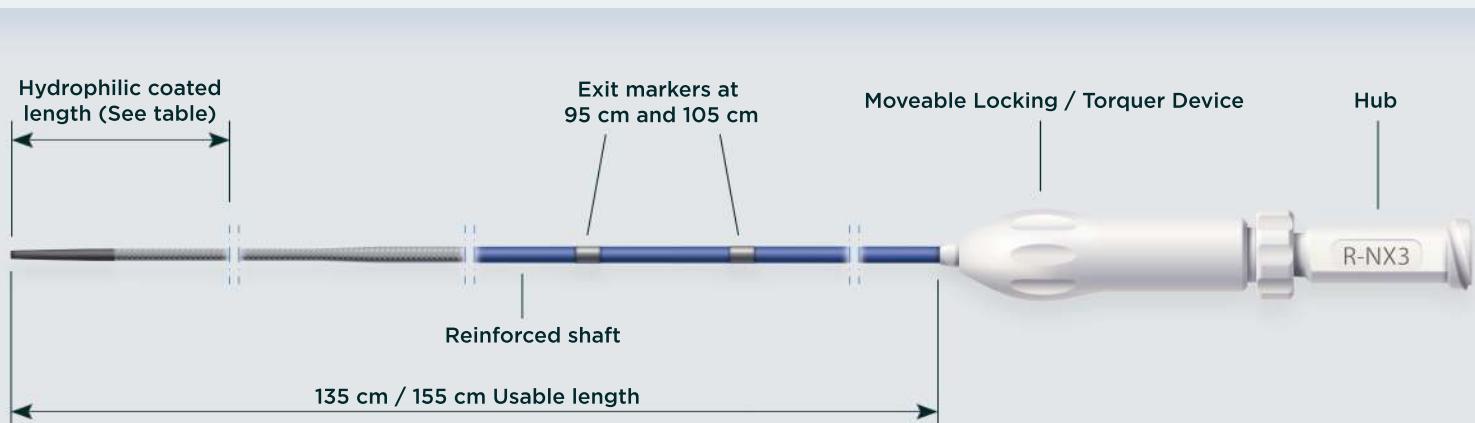

UNIQUE HYBRID GW-SHAFT LOCK

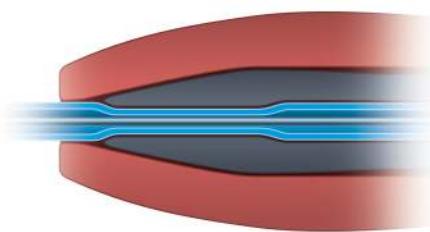

NX31413525 & NX31415560



NX61413525 & NX61415560



IMPROVES PRIMARY WIRING AND PROCEDURAL SUCCESS RATES<sup>1</sup>

PRO X CROSS WITH SOFT HIGH PENETRATION TIP

PRO X MOSQUITO TIP WORKHORSE MICRO CATHETER

Technical specifications	NX31413525 (A-NX3)	NX31415560 (R-NX3)	NX61413525 (A-NX6)	NX61415560 (R-NX6)
Guidewire size	0.014"	0.014"	0.014"	0.014"
Usable length	135 cm	155 cm	135 cm	155 cm
Hydrophilic coating	NDurance	NDurance	NDurance	NDurance
Hydrophilic coating length	25 cm	60 cm	25 cm	60 cm
Proximal shaft outer diameter	3.0F	3.0F	2.6F	2.6F
Distal shaft outer diameter	2.0F	2.0F	2.3F	2.3F
Proximal shaft inner diameter	0.52 mm	0.52 mm	0.52 mm	0.52 mm
Distal shaft inner diameter	0.45 mm	0.45 mm	0.48 mm	0.48 mm

<sup>1</sup>Wilson. S, Maeremans. J, Walsh. S, Hanratty. C, Gessner. M.M, Dens. J, Christiansen. E, Bufo. A, Spratt. J; The first clinical experience with a novel "locking" microcatheter in chronic coronary total occlusions. *Eurointervention* 2017;12:e1-e6

for more information  
[WWW.IMDS.NL](http://WWW.IMDS.NL)

Please see the Instructions for Use for a complete listing of the indications, contraindications, warnings and precautions.

Caution: Federal Law (U.S.) restricts this device to sale by or on the order of a physician.  
 NHancer™ is a trademark of IMDS.

© IMDS 2019 ITM150171 R9.0

Ceintuurbaan Noord 150  
 9301 NZ Roden  
 The Netherlands  
 sales@imds.nl

Phone +31(0)50 8200230  
 Fax +31(0)50 8200231

